

## **MEASUREMENT OF VERY SMALL CHANGES OF OBJECT POSITION USING SPECKLE CORRELATION METHOD**

**Milan Navrátil, Vojtěch Křesálek, Radek Slušík  
Tomas Bata University in Zlín, Faculty of Applied Informatics  
Nad Stráněmi 4511, 76005, Zlín, Czech Republic**

### **ABSTRACT**

*The paper deals with measurement of very small changes of object position using speckle correlation method. An object translation measurement is very often measured deformation tensor components. The most measuring method is based on direct contact with the object, which can be often destructive. Presented contactless method uses statistical approach which means computation of the cross-correlation function of the two speckle patterns recorded before and after object translation.*

**Keywords:** speckle, laser, contactless measurement, change of object position

### **1. INTRODUCTION**

Problems of contactless optical measurement of translations rotations and deformations achieved two significant phases up to now. The first one occurred in 50<sup>th</sup> and it was primarily characterized by photoelasticity. The second one came in 70<sup>th</sup> and it was characterized by holographic interferometry and speckle holography method. However, not a single one method from these due to their complexity found wider use in practice. Recently, in times of turbulent development of computer techniques, light sources and detectors the restoration of methods using coherency grain arises. Above all, methods using cross-correlation function of two coherency grain intensity fields which are measured before and after surface change of an object. From the point of contemporary mechanics, main advantages of mentioned methods are non-contacts measurement, variability, possibilities of mechanization and also automation of measured data processing.

### **2. THEORETICAL ASPECTS**

This optical method is based on speckle phenomenon which is also often called coherency grain. It occurs during

- reflection of coherent light from coarse interface
- pass of coherent light through coarse interface
- pass of coherent light through environment with random fluctuations of refractive index

Physics of this phenomenon is interference of light waves originating either from number of microscopic surfaces which are considered on object's surface during reflection or from dispersion on randomly distributed particles during pass. As a result, a visible figure (speckle field) consisting of light and dark stains which is possible to observe on a shade located whenever in front of the lens (during reflection) and located behind the lens during pass. Size and appearance of grains depend on coherency stage of incident light, on its polarization and also on properties of dispersing environment [1], [2]. Change of speckle field can be quantitatively described with change of maximum position of statistical cross-correlation function between two intensity fluctuations of coherency grain from object before and after its deformation.[3]

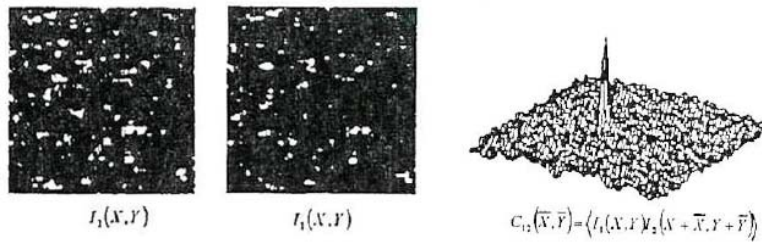


Figure 1. Illustration of speckle field with corresponding cross-correlation function.

In Figure 1 can be seen two photos of speckle field before and after translation and corresponding cross-correlation function. During object deformation, the correlation has always non-zero position and it represents an extent of change of measured object position. Simultaneously, value of maximum is decreasing which is caused by change of speckle field structure during deformation.

### 3. USED INSTRUMENTS

#### AXIS 221 Network Camera

It is a high performance camera for round-the-clock surveillance over IP networks. The camera provides high quality images (up to 45 frames per second in VGA resolution - 640 x 480 pixels) under all lighting conditions, which makes it an ideal solution for indoor/outdoor applications.

#### JDS Uniphase Helium Neon Laser

It features a patented close-cathode design that provides improved thermal stability for superior beam pointing and power stability, as well as a patented field concentrator design that enables fast turn-on. The precisely aligned cylindrical housing on the JDS Uniphase HeNe laser and electrical interconnect system simplify system integration. JDS Uniphase units are rugged enough for the most demanding applications.

#### M110 Compact Micro-Translation Stage

It is an ultra-high resolution (0.007  $\mu\text{m}$ ) motorized translation stage providing linear motion of 5 mm in an extremely compact package. They feature a precision leadscrew with sub-micron resolution and precision linear ball bearings guaranteeing  $<0.5 \mu\text{m}$  straightness of travel.

### 4. EXPERIMENTAL

Measuring system consists of source of coherent light which is focused on a rough part of measured object, the camera watching coherence grain and the computer which evaluates video data (Figure 2).

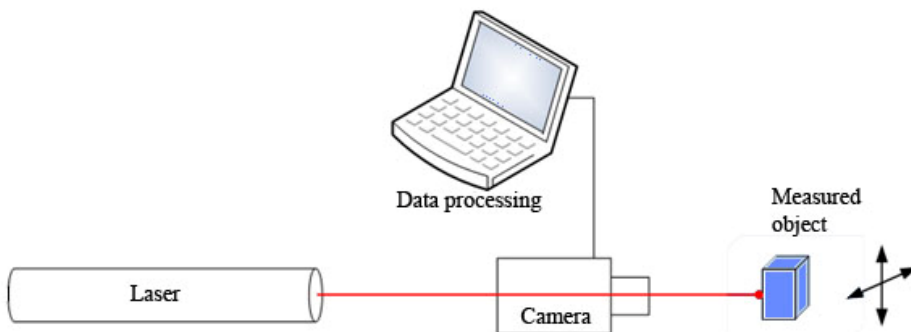


Figure 2. Scheme of measuring system.

At first, a verification of measured method was accomplished, so some simplifications were considered. We assumed only motion in horizontal or vertical line. Due to this fact, only one row or column of the video data was taken for evaluation of intensity fluctuations of coherency grain. In this paper, we only dealt with evaluation of motion in vertical line so that one column of pixels was

processed. To verify measuring method, the micro-translation stage was used and it was controlled by PI Mercury software via RS232 interface. Translation change of the stage was accomplished only for linear vertical line, length of translation was 2 mm, velocities were chosen 17.5, 35, 70, 140, 280, 560 and 1120  $\mu\text{m/s}$ . Lens of Axis 221 was removed and the camera was properly adjusted in order that coherence field which is reflected from measured object surface can drop on the CMOS sensor. The camera was connected with the coputer via RJ-45 interface, frame rate was set at 30 frames per second.

Essential algorithms in Matlab were created for complete evaluation of measured data, such as program for calculation of: presence time of speckle, speckle size, intensity of speckle field, distance in pixels and velocity of motion. **Presence time of speckle** is an average period of time when individual speckle originates and then lasts. This parameter defines range of measuring method and also means the longest permissible time between two neighbouring evaluated frames (see Figure 3). **Speckle size** is an average size of speckle in evaluated column of CMOS sensor. This parameter represents sensitivity of the method (see Figure 4).

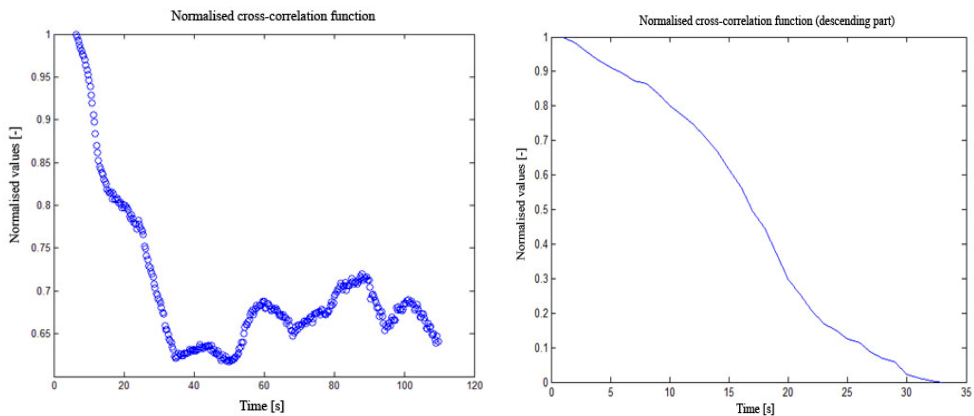


Figure 3. Normalised cross-correlation function (left). On the right, only descending part of curve is normalized, it represents presence time.

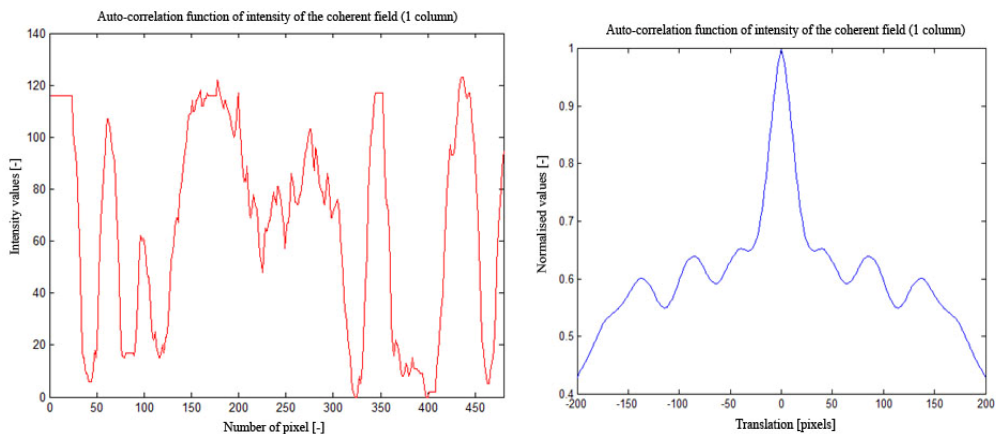


Figure 4. Normalised cross-correlation function (left). On the right, only descending part of curve is normalized, it defines speckle size.

Following table shows results of measuring process where object's known velocity was measured.

Table 1. Measured values of velocity of the moving object.

Reference velocity	Evaluated part of video data		Measured velocity	Difference of velocities	
	[ $\mu\text{m/s}$ ]	[step frame]		[frame number]	[ $\mu\text{m/s}$ ]
17,5	50	110-1800	20,4	2,9	17
35	25	100-800	43,4	8,4	24
70	15	100-400	83,7	13,7	20
140	8	200-380	172,2	32,2	23
280	4	30-130	333,1	53,1	19
560	2	40-90	674,5	114,5	20
1120	1	48-53	1359,0	239,0	21

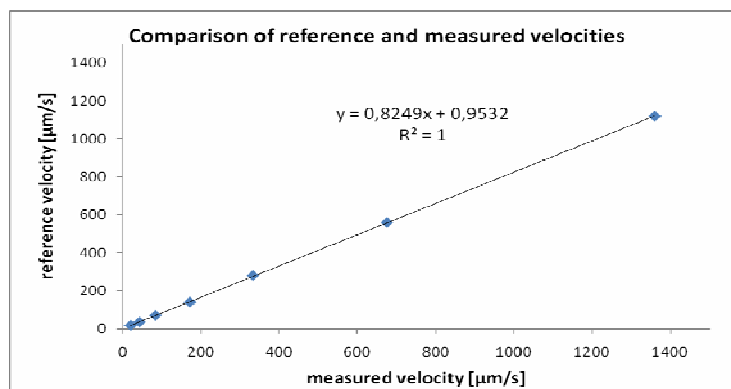


Figure 5. Dependence of reference velocity on measured one.

## 5. CONCLUSION

Method position change measurement of the bodies by using speckle phenomena is from the point of view of nowadays metrology very interesting method, because it is a noncontact method. Unfortunately, this method has some specifics, which essentially limits its using in practice. At the moment of measuring, there must be kept specific conditions and their breach causes a decrease of sensitivity or using of the method itself. Scanned surface should be straight, without any deformation and its roughness must have a value to produce a laser speckle phenomena. From obtained results is evident, that measuring error is about 20 percent but after simple correction it can be very well used for measuring of velocity (Figure 5). If there are kept the conditions mentioned above this method achieves very accurate values of measured data

## 6. ACKNOWLEDGEMENT

This work was accomplished with financial support by Research Projects of the Ministry of Youth, Education and Sports of the Czech Republic: MSM 7088352102.

## 7. REFERENCES

- [1] Rajpal S. Sirohi, Speckle metrology, CRC Press, 1993, ISBN 0824789326.
- [2] Horváth, P., Šmíd, P., Wagnerová, P., Hrabovský, M.: Non-contact measurement of small deformation of object by means of the speckle correlation method, *Jemná mechanika a optika*, 3/2005.
- [3] Hrabovský, M., Bača, Z., Horváth, P.: *Koherenční zrnitost v optice*, UPOL Olomouc, 2001, ISBN 80-244-0286-6.
- [4] Hariharan, P.: *Optical Interferometry*, Academic Press, Sydney, 1985.
- [5] Yamaguchi, I.: Real-Time Measurement of in-Plane Translation and Tilt by Electronic Speckle Correlation. *Jpn. J. Appl. Phys.* 19 (1980) L131.